



Replacement Drawings
SN 10/798,299

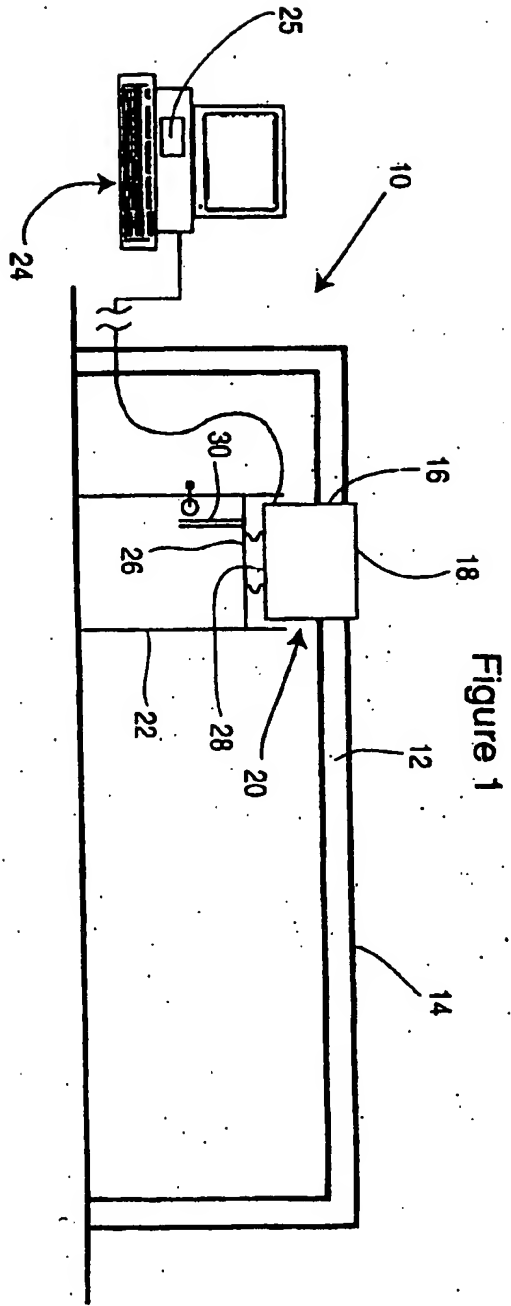


Figure 1

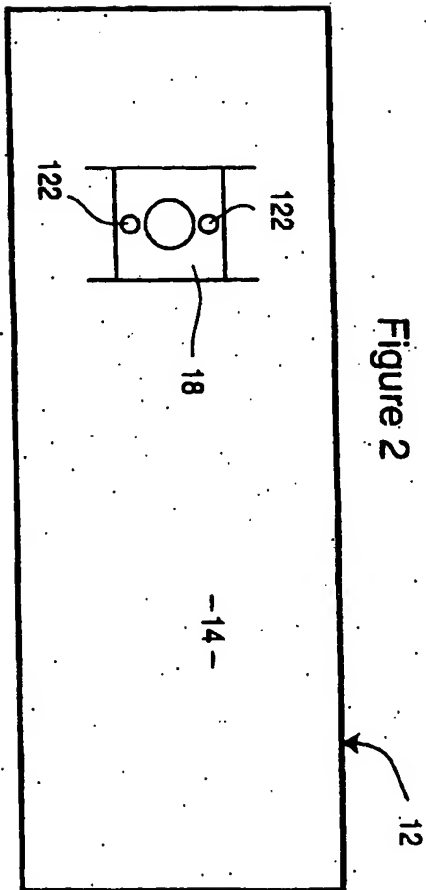


Figure 2

Figure 3

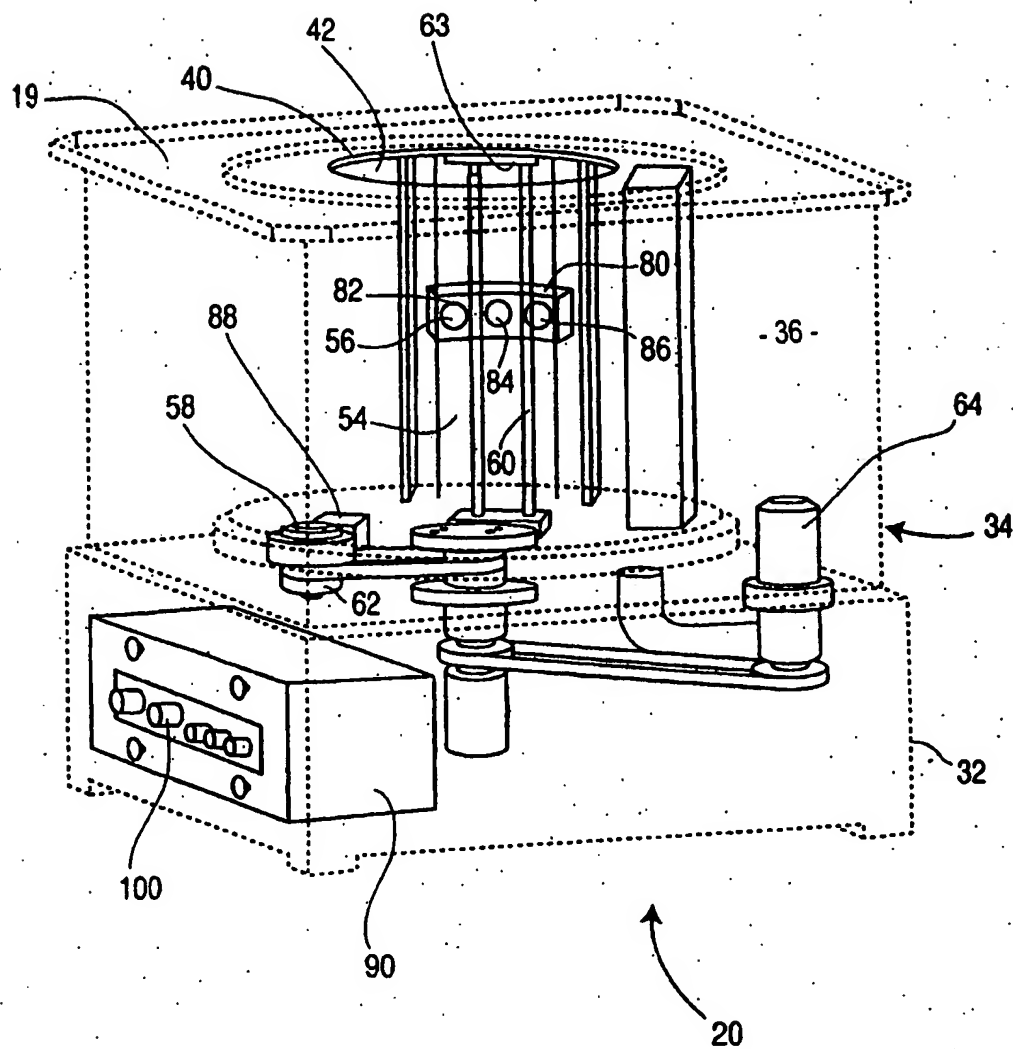


Figure 4

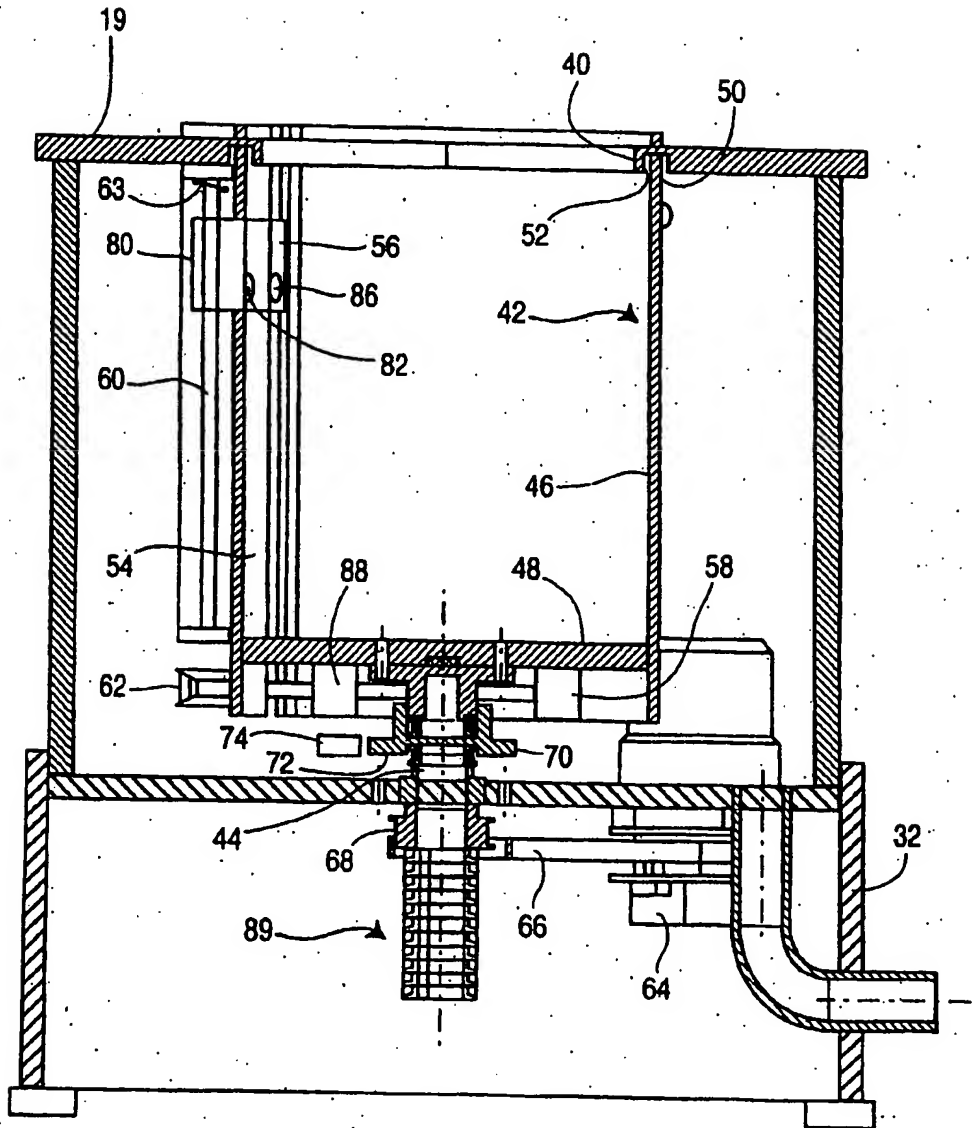


Figure 5

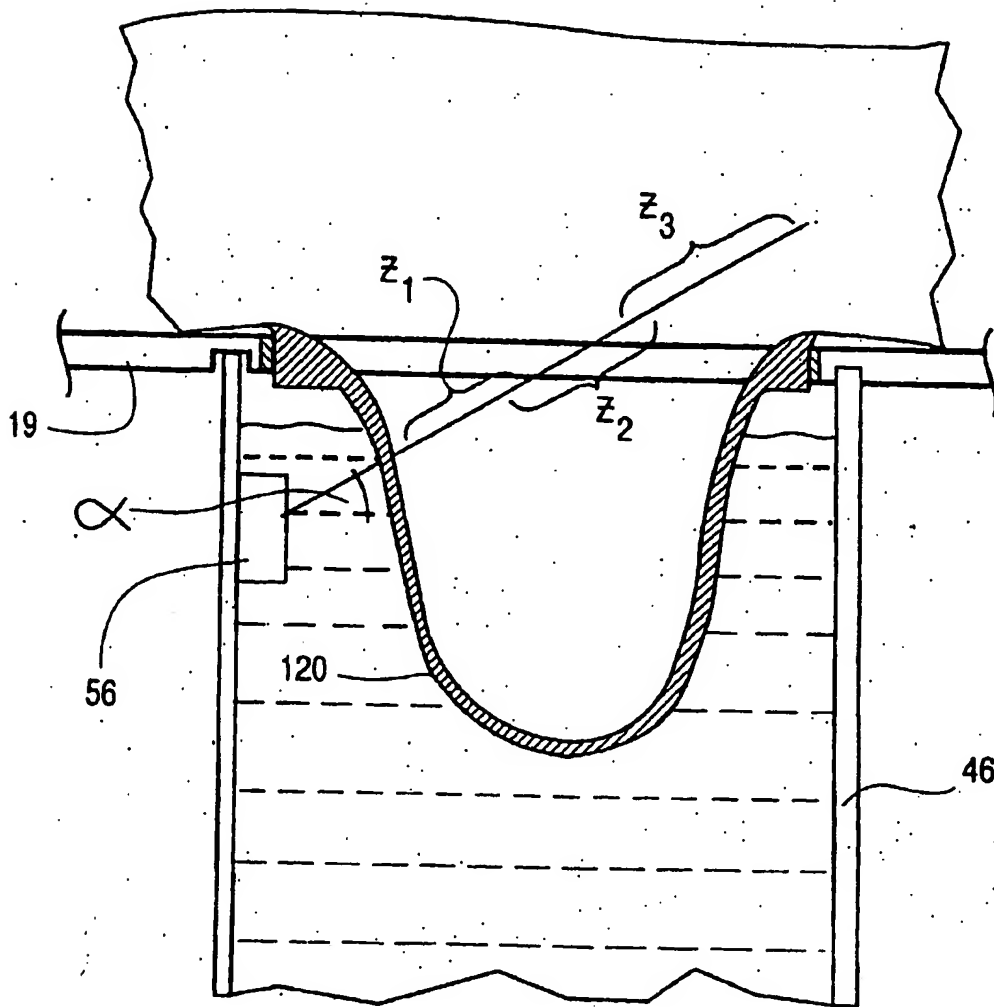


Figure 6

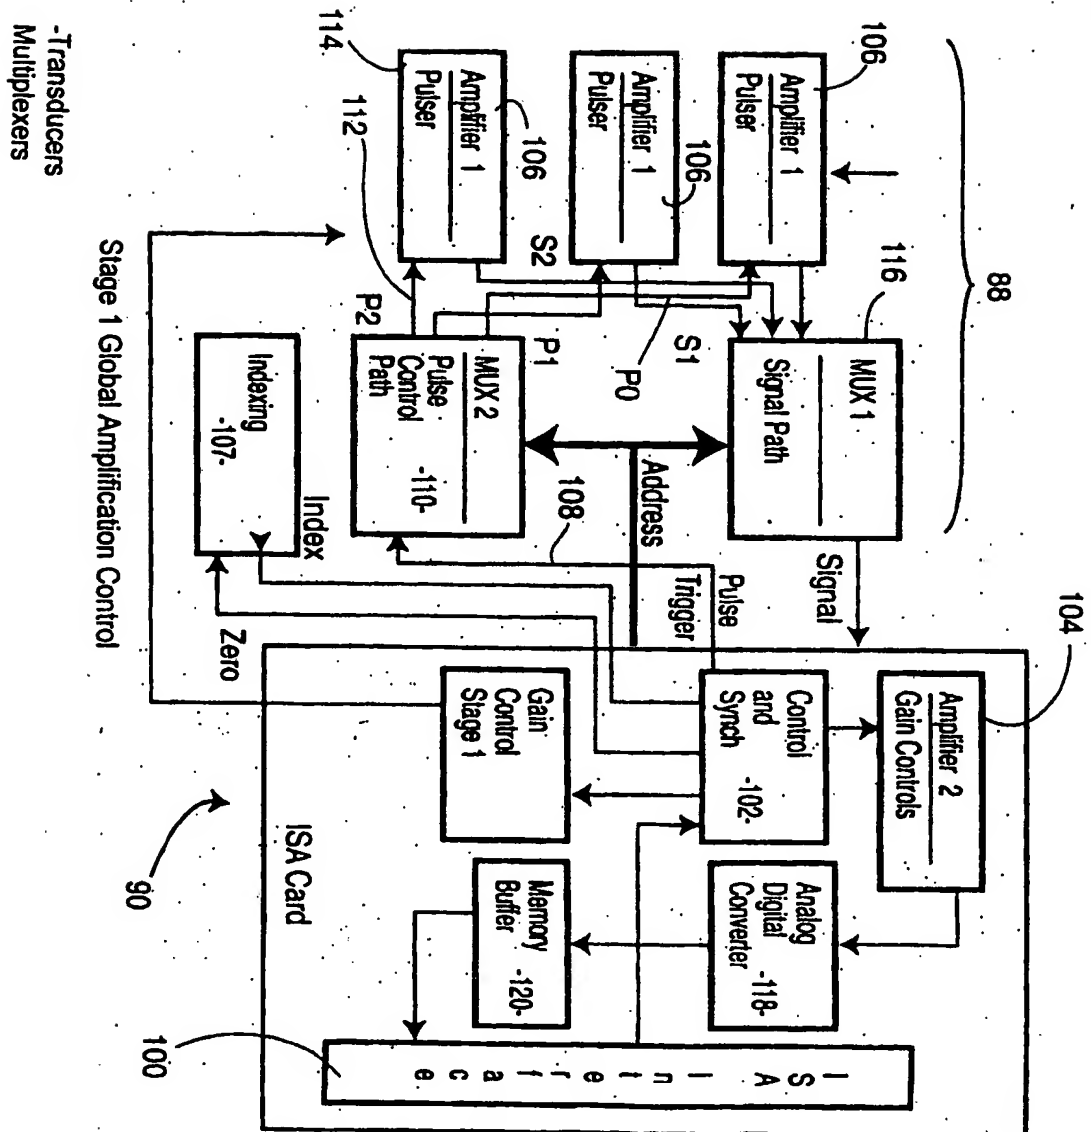


Figure 7

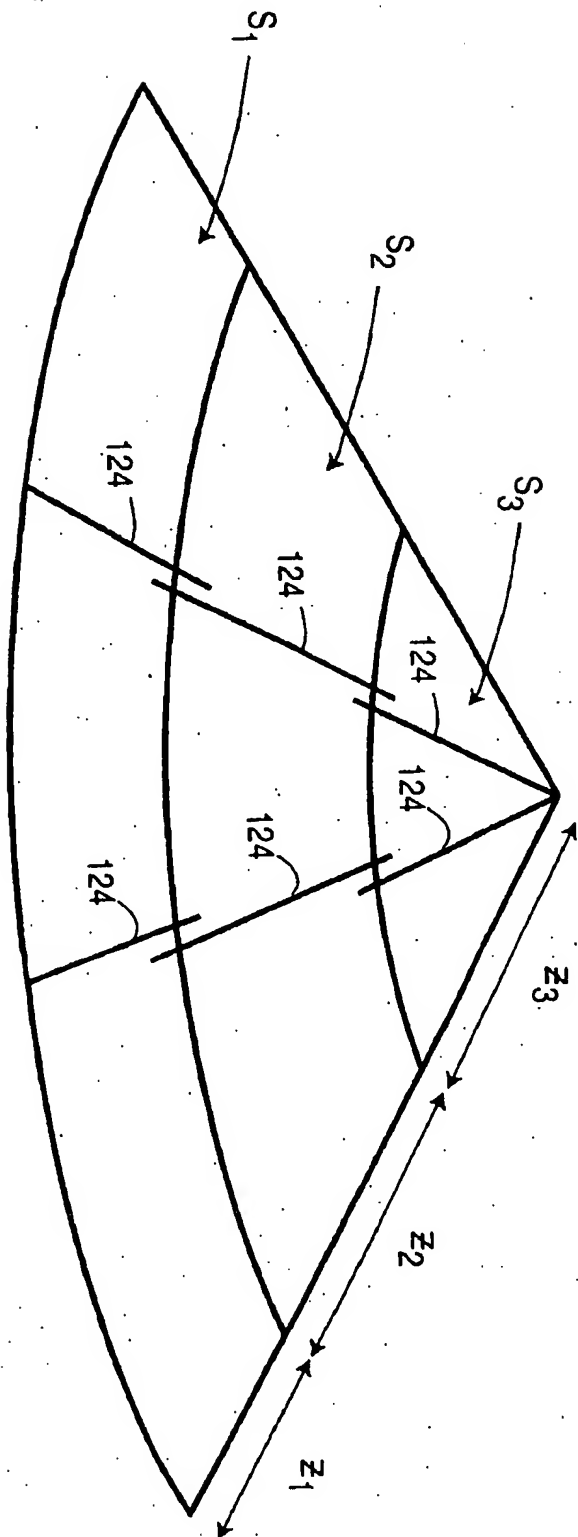


Figure 8

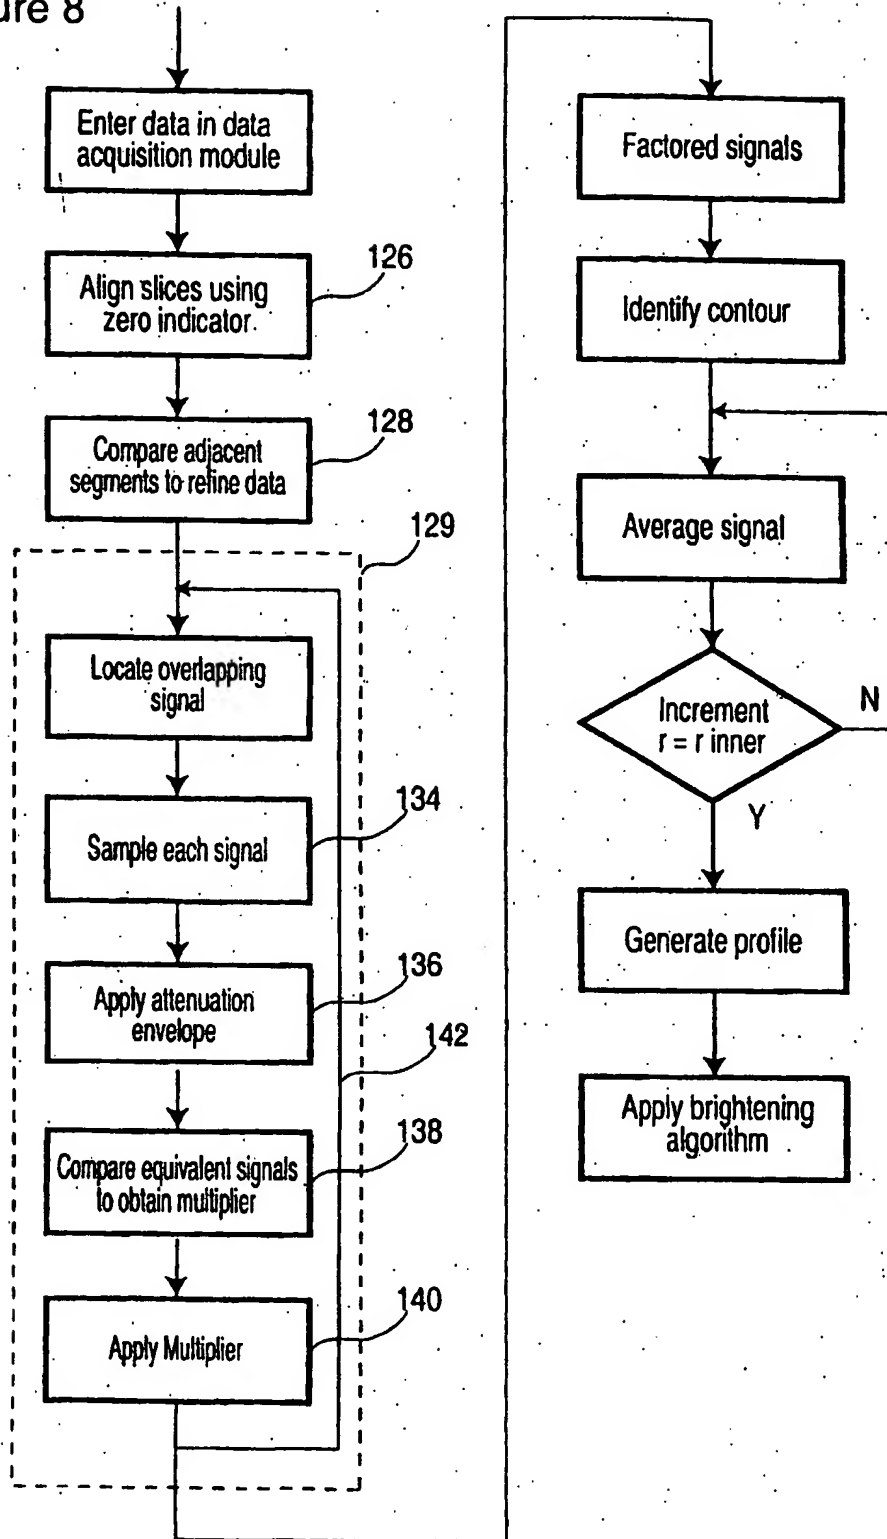


Figure 9

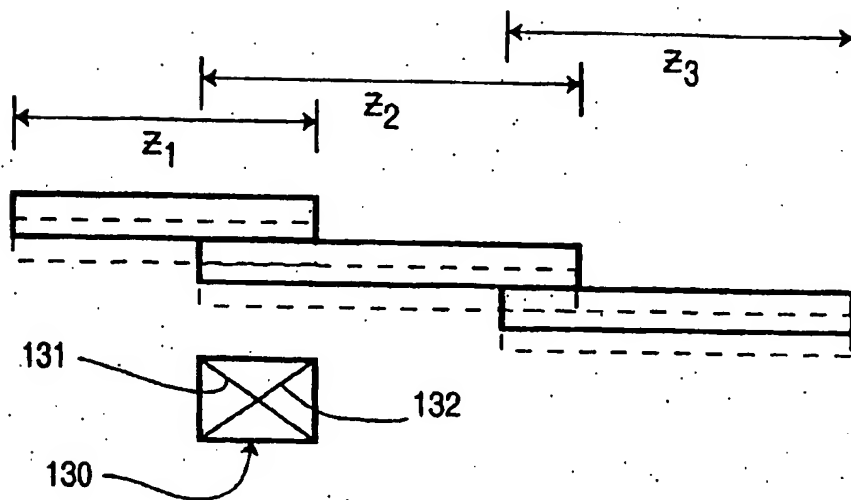


Figure 10

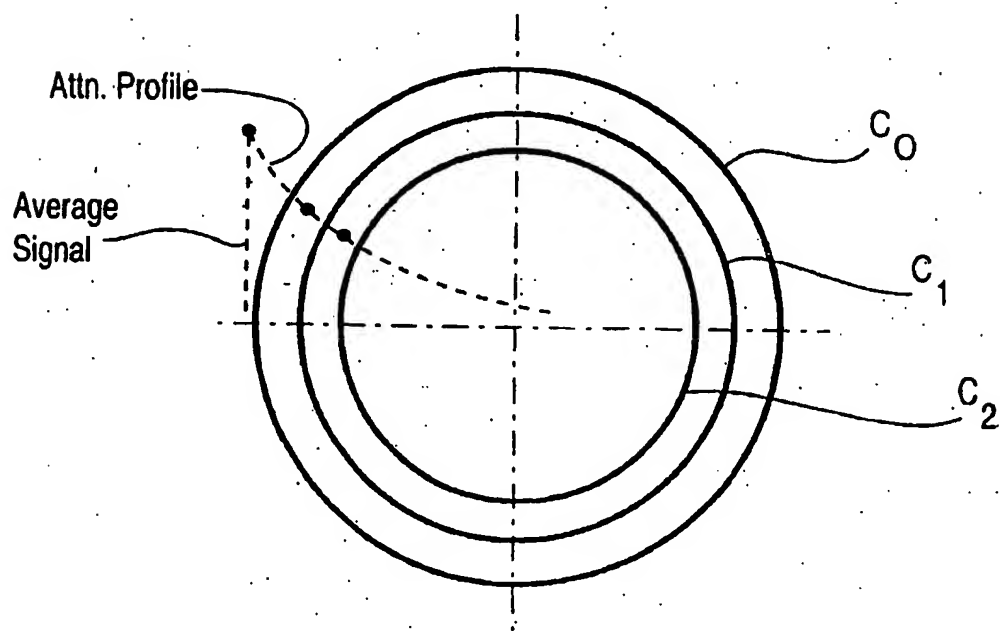


Figure 11

The interface is divided into several functional areas:

- Top Bar:** Contains buttons for "MediPattern", "Registration", "Cabinet", "Scan", "MPR", and "Logout".
- Left Panel (200):**
 - Acq. Params:** Includes "Recon Params" and "Saved Settings".
 - USG [USG Scanner 5]:** A dropdown menu.
 - Device Settings:** Includes "Step Size (0.1mm)" with a slider, "Vertical Count" with a slider, and "Vertical Start (0.1mm)" with a slider.
 - Card Settings:** Includes "Amplifier" (17VV), "Sampling" (20 MHz), and "Breast" (Right).
 - Preview/Scan Mode:** Includes a "Quality" dropdown and a "Size" dropdown (Size B).
 - Power:** Includes "On", "Off", and "Go Up" buttons.
 - Transducer Preamp:** Includes a slider and a "Vertical Mirror" checkbox.
 - Cine Controls:** Includes "Cine Type" (Yolo, Loop), "Speed (fps)" (5), "Play", and "Stop" buttons.
 - Bottom Left:** Includes "Preview", "Scan", "RECON", "Delete", and "Save" buttons.
- Right Panel (202):**
 - Acquisition / Reconstruction:** A toggle switch.
 - Folder D: 1010 Name:** A text field.
- Main Display Area (204):** A large rectangular area for the ultrasound image, with a vertical scrollbar on the right side.